

# DEVITA BRT

BIORESONANCE TELEMETRIC CORECTION

DIGITAL DEVICE FOR ENDOGENOUS BIORESONANCE CORRECTION OF  
THE BODY

## MANAGE YOUR HEALTH

AUTOMATED PROFESSIONAL METODOLOGY FOR DOMESTIC USE



PERSONAL ADJUSTMENT OF  
THE BODY



ACTIVATION OF THE ADAPTION  
ABILITIES



QUICKER RECOVERY



# DEVITA BRT

BIORESONANCE TELEMETRIC CORRECTION

MANAGE YOUR HEALTH

REASONABLE DIMENSIONS AND WEIGHT

RECHARGEABLE BUILT-IN BATERIES

UNLIMITED NUMBER OF USERS

COMPATIBLE WITH SEVERAL PROGRAMS OF DEVITA RITM AND DEVITA ENERGY

DURATION OF ONE SESSION IS 20 MINUTES





# DEVITA BRT


BIORESONANCE TELEMETRIC CORRECTION

## HOW IT WORKS

**BIORESONANCE TELEMETRY (BRT)** – it is improvement of health state utilizing own electromagnetic oscillations of the patient.

### DEVITA BRT INVERSIVE MODE

recording, strengthening and turning upside-down the pathogenic electromagnetic oscillations of the body; creates neutralizing interaction of pathogenic and correcting oscillations and restores healthy physiological oscillations of the patient's organism.

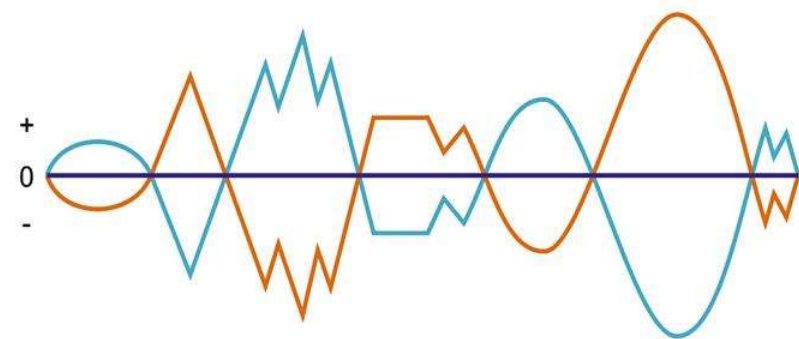

- Pathogenic oscillations
- Correcting oscillations (pathogenic oscillations inverted on 180°)
- Physiological oscillations

**INVERSION** (derives from the Latin word *Inversio* – turning over, upside-down) – the method invented by German Doctor Franz Morell and Engineer Erich Rasche in the middle of XX Century.



# DEVITA BRT

BIORESONANCE TELEMETRIC CORRECTION

## BIOLOGICAL FUNDAMENTALS OF INFLUENCE



EFFICIENTLY



SAFELY




PHYSIOLOGICALLY



CONVENIENTLY

Reading the electromagnetic oscillations of a person and health improving influence is implemented through the bio-active points of the body located within the zones of projection of the organs on the skin of arms and feet

SKETCH FOR THE DEVICE CONNECTION

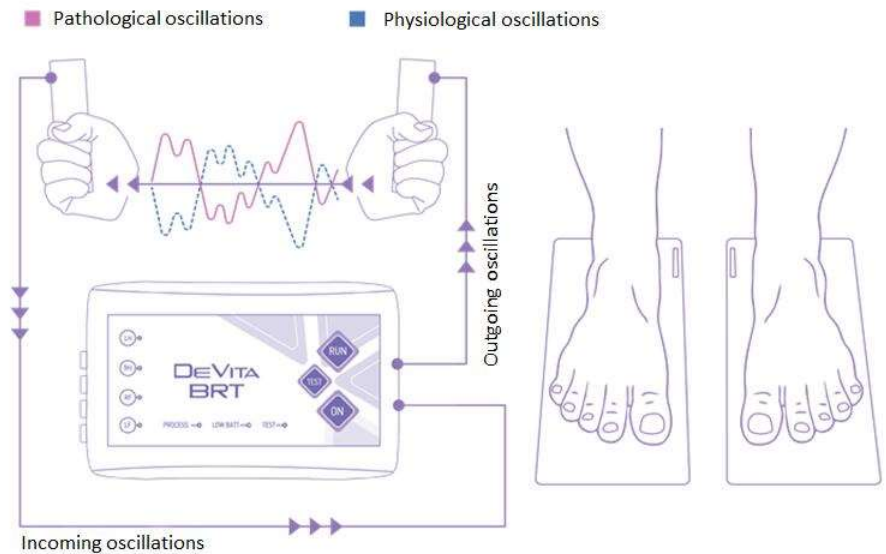

# DEVITA BRT

BIORESONANCE TELEMETRIC CORRECTION

## AUTOMATED PROFESSIONAL METHODOLOGY



EASY TO CONNECT



AUTOMATIC PROGRAM



EASY TO USE

**STEP 1** Reads the own electromagnetic oscillations of the body.

**STEP 2** Inverts and neutralizes pathogenic/disharmonious oscillations; strengthens physiological/harmonious oscillations.

**STEP 3** Returns the physiological/harmonious oscillations to the human body.





# DEVITA BRT

BIORESONANCE TELEMETRIC CORRECTION

## THE NECESSARY CONDITIONS FOR AN EFFECTIVE HEALTH IMPROVING SESSION



24 HOURS BEFORE THE SESSION EXCLUDE SMOCKING, CONSUMPTION OF ALCOHOLIC BEVERAGES AND COFFEE



PRIOR THE SESSION IT IS RECOMMENDED TO IMPLEMENT ALL-ROUND ESTIMATION OF THE BODY STATE UTILIZING OUR DEPULS+ COMPLEX



THE SESSION LOCATION MUST NOT BE IN GEO-PATHOGENIC ZONE AND/OR HAVE ANY HARMFUL ELECTROMAGNETIC FIELDS



THE OPERATING ELECTRIC APPLIANCES MUST NOT BE CLOSER THAN 0.5 M FROM THE PLACE OF THE TREATMENT



USE THE CLOTHES MADE OF NATURAL FABRICS TO AVOID ACCUMULATION OF STATIC ELECTICITY



FOR BETTER CONTACT OF THE PALMS AND FEET WITH ELECTRODES PLEASE MOISTEN THE ELECTRODE SURFACE WITH A WET NAPKIN NOT CONTAINING ALCOHOL OR PERFUME

# DEVITA BRT

BIORESONANCE TELEMETRIC CORRECTION

THE WAY OF COMBINED USE OF **DEVITA** DIGITAL DEVICES FOR PERFECT HEALTH IMPROVEMENT

## DEVITA RITM MINI

### Program:

- Active protection
- Anti-stress
- Blood circulation regulation
- Digestion
- Detoxification



## DEVITA ENERGY MINI

### Program:

- Energy

**STEP 1** CHOOSE ON THE DIGITAL DEVICE **DEVITA RITM MINI** or **DEVITA ENERGY MINI** ONE OF THE SUGGESTED PROGRAMS

**STEP 2** WHEN READY FOR THE BIORESONANCE TELEMETRIC CORRECTION SESSION TURN-ON ONE OF THE PROGRAMS YOU HAVE CHOSEN

NEVER USE BOTH **DEVITA RITM MINI** AND **DEVITA ENERGY MINI** DEVICES SIMULTANEOUSLY!